
14. Total RNA Extraction from Fish and Clam



Total RNA Extraction from Body Cavity Fluid of Fish

Protocol

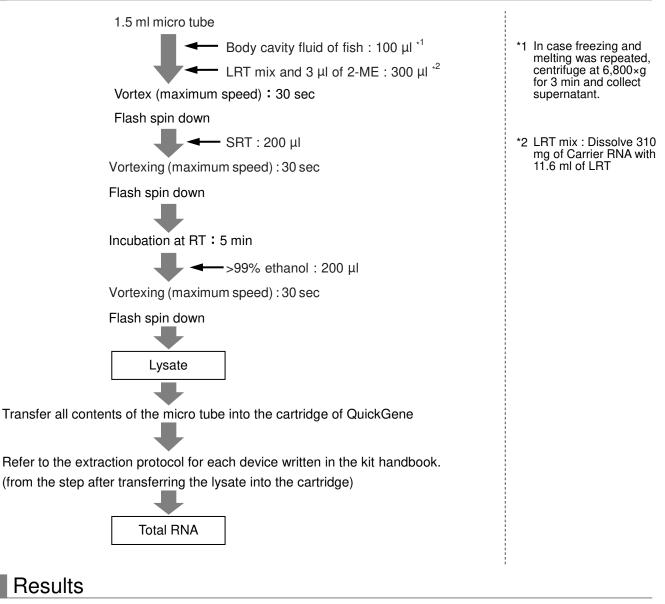

Amount of body cavity fluid	A260/280
100 μl	1.6

Common protocol is usable for the following

No Data

Depending on sample and storage conditions, nucleic acid may not be extractable. Therefore, we cannot guarantee accurate data. The extracted nucleic acid contains unintended acid (ex: when extracting DNA, RNA is also extracted).


KURABO



RD-2

Total RNA Extraction from Fin of Killifish

Protocol

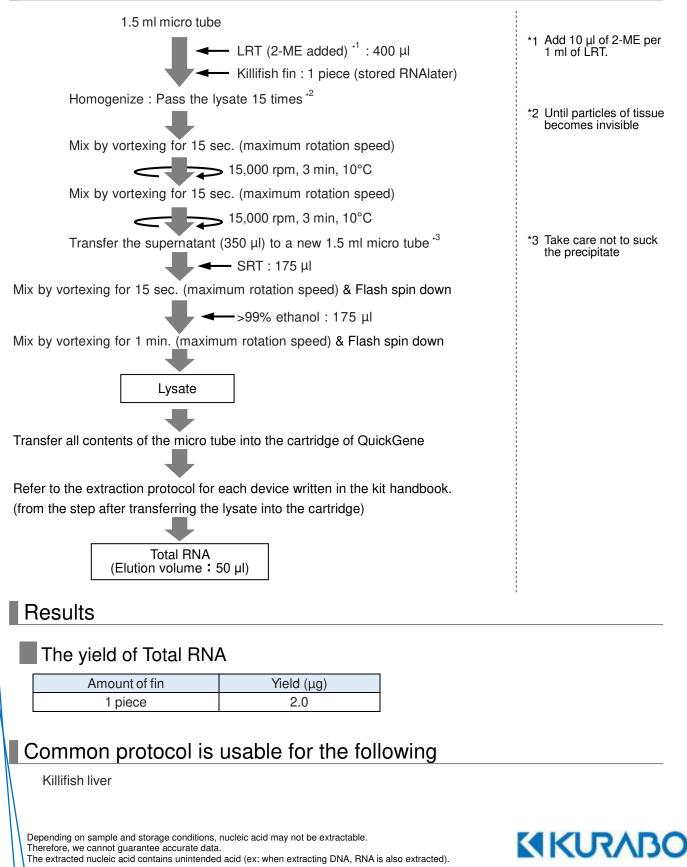




RD-3

Total RNA Extraction from Liver of Killifish

Protocol

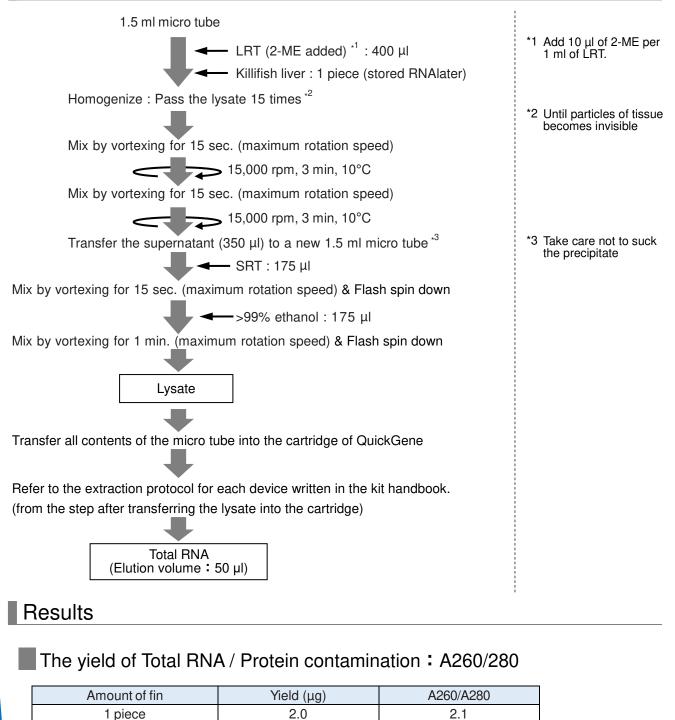

Common protocol is usable for the following

Killifish fin

Depending on sample and storage conditions, nucleic acid may not be extractable. Therefore, we cannot guarantee accurate data. The extracted nucleic acid contains unintended acid (ex: when extracting DNA, RNA is also extracted).

